




# HiTech Bed

## QUICK REFERENCE SHEET

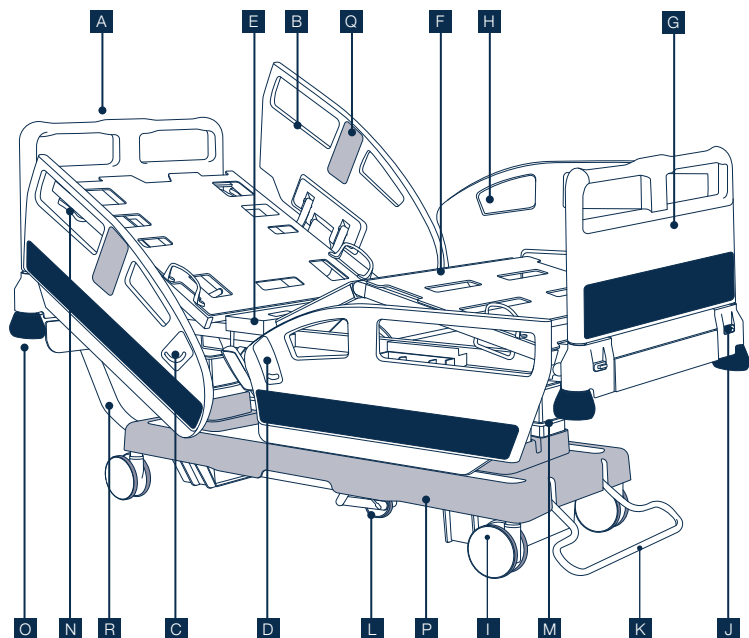

### BED'S COMPONENTS

A	Removable curved headboard	J	Unlocking headboards and footboards
B	Backrest section side rail	K	Centralised braking system
C	Backrest tilt angle indicator	L	5 <sup>th</sup> wheel
D	Trend & Reverse trend tilt angle indicator	M	Lifting columns
E	Sheet steel central section	N	Emergency CPR
F	HPL mattress platform	O	Protection disc
G	Removable curved footboard	P	Cover frame
H	Leg section side rail	Q	Membrane controls
I	Wheels Ø150 mm.	R	Anchored headboard

### OTHER FUNCTIONS

#### Side Rails (1):

- Raising the rail: Pull the rail upwards until it is immobilised in the highest position.
- Lowering the rail: Pull the handle found underneath the rail outwards. The rail will automatically lower.


#### Emergency CPR (2):

- Activate either of the two levers located under the headrest module, accompanying it in turn as it


lowers.

#### Centralised braking system (3):



- Braking the bed: Pedal in low position.
- Moving the bed: Pedal in intermediate position.
- Activating 5th or Steering wheel: Pedal in raised position.




Raising the rails

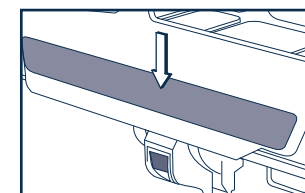


Lowering the rails

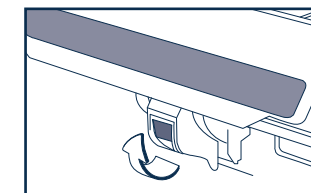


Emergency CPR



Brake



Free movement



Steering or 5th wheel

### CLEANING

Daily cleaning and disinfection with soapy water:

- Rails. Head board. Foot board.

Cleaning and disinfection after a patient leaves or before a transfer:

- Mattress platform area. Chassis of the bed.

Thorough cleaning and disinfection every two months:

- Support and lifting area of the bed.

### MAINTENANCE

Always check the correct state of:

- Electrical wiring
- Wheels.
- Braking mechanisms.

www.pardo.es


TECHNICAL SERVICE CENTRE

(+34) 976 300 033


For more information, please consult the use and maintenance manual.




# CONTROLS

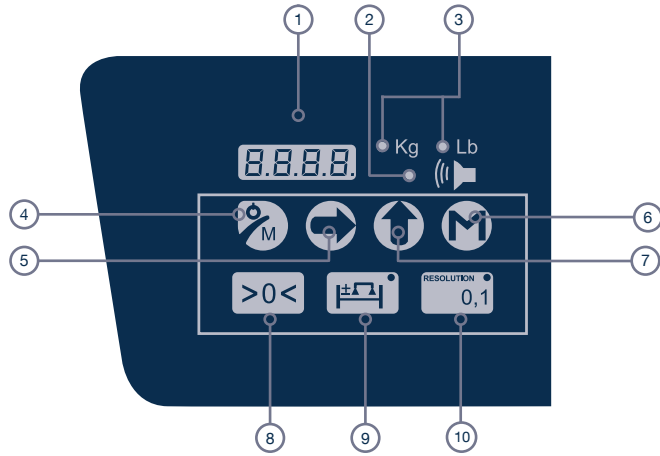


Weighing system

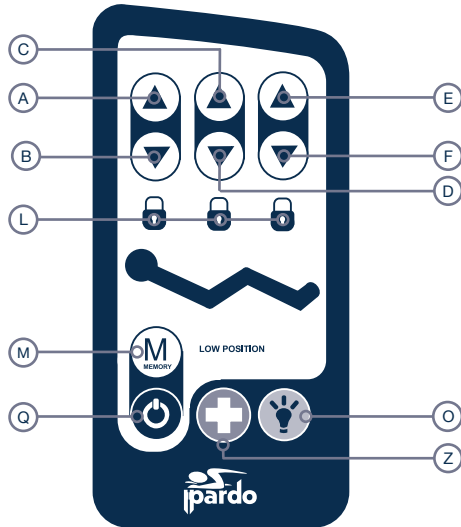

Membrane control

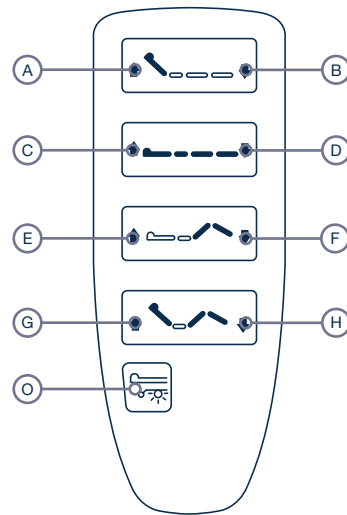

Patient control with light

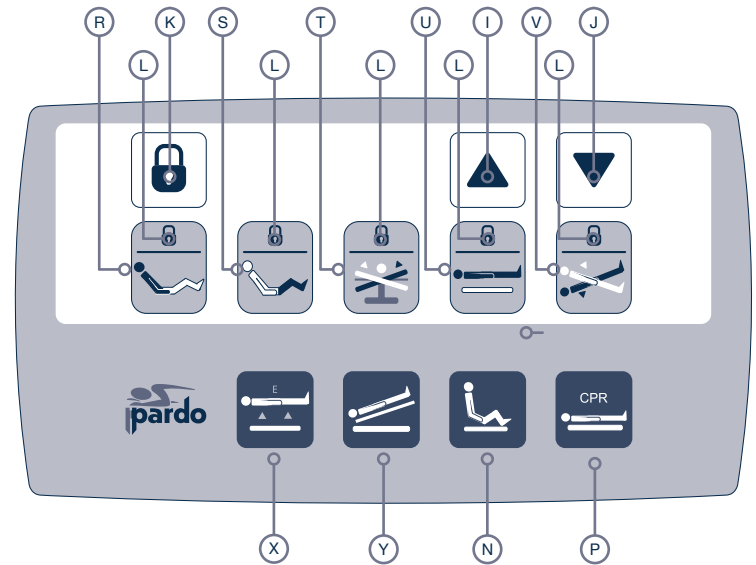

Nursing control

## INSTRUCTIONS OF USE

A	Rise backrest	M	Memory button	Z	Nurse call
B	Lower backrest	N	Cardiac chair position	1	Digit screen
C	Rise mattress platform	O	Light	2	Alarm indicator
D	Lower mattress platform	P	Emergency CPR	3	Unit indicator
E	Rise legrest	Q	On/Off Button (to active membranes)	4	On/off key - menu - data validation
F	Lower legrest	R	Backrest selector	5	"Right" key
G	Rise all sections simultaneity ( <i>autocontour</i> )	S	Legrest selector	6	"Memory" key
H	Lower all sections simultaneity ( <i>autocontour</i> )	T	Tilting selector	7	"Up" key
I	Trend	U	Mattress platform selector	8	"Back to zero" key
J	Reverse trend	V	Trendelenburg / Reverse trendelenburg selector	9	"Auto-compensation" key
K	Locking movements	X	Explorer Position (Maximum height)	10	Resolution key
L	Indicator Led of locked movements	Y	Emergency Trend position		



### SAFETY WARNINGS

- The maximum duration of a continuous manoeuvre should not exceed 2 minutes, as damage may be caused to the equipment.
- Before raising and lowering the moving parts of the mattress platform, with the other parts of the bed or accessories, it is essential to check that there are no obstacles between them.
- The Trendelenburg and reverse Trendelenburg movement should always be performed under medical supervision.
- When the bed is in extended position, do not sit or lean on the foot part of the bed, since it may cause a bed dump.
- Do not use CPR bilateral actuating levers to raise the backrest of the bed, it may cause raise motor breakdown and makes a bed dysfunction.

